


MARC-43 (CHIME) Study – Algorithm for Obtaining Research Blood

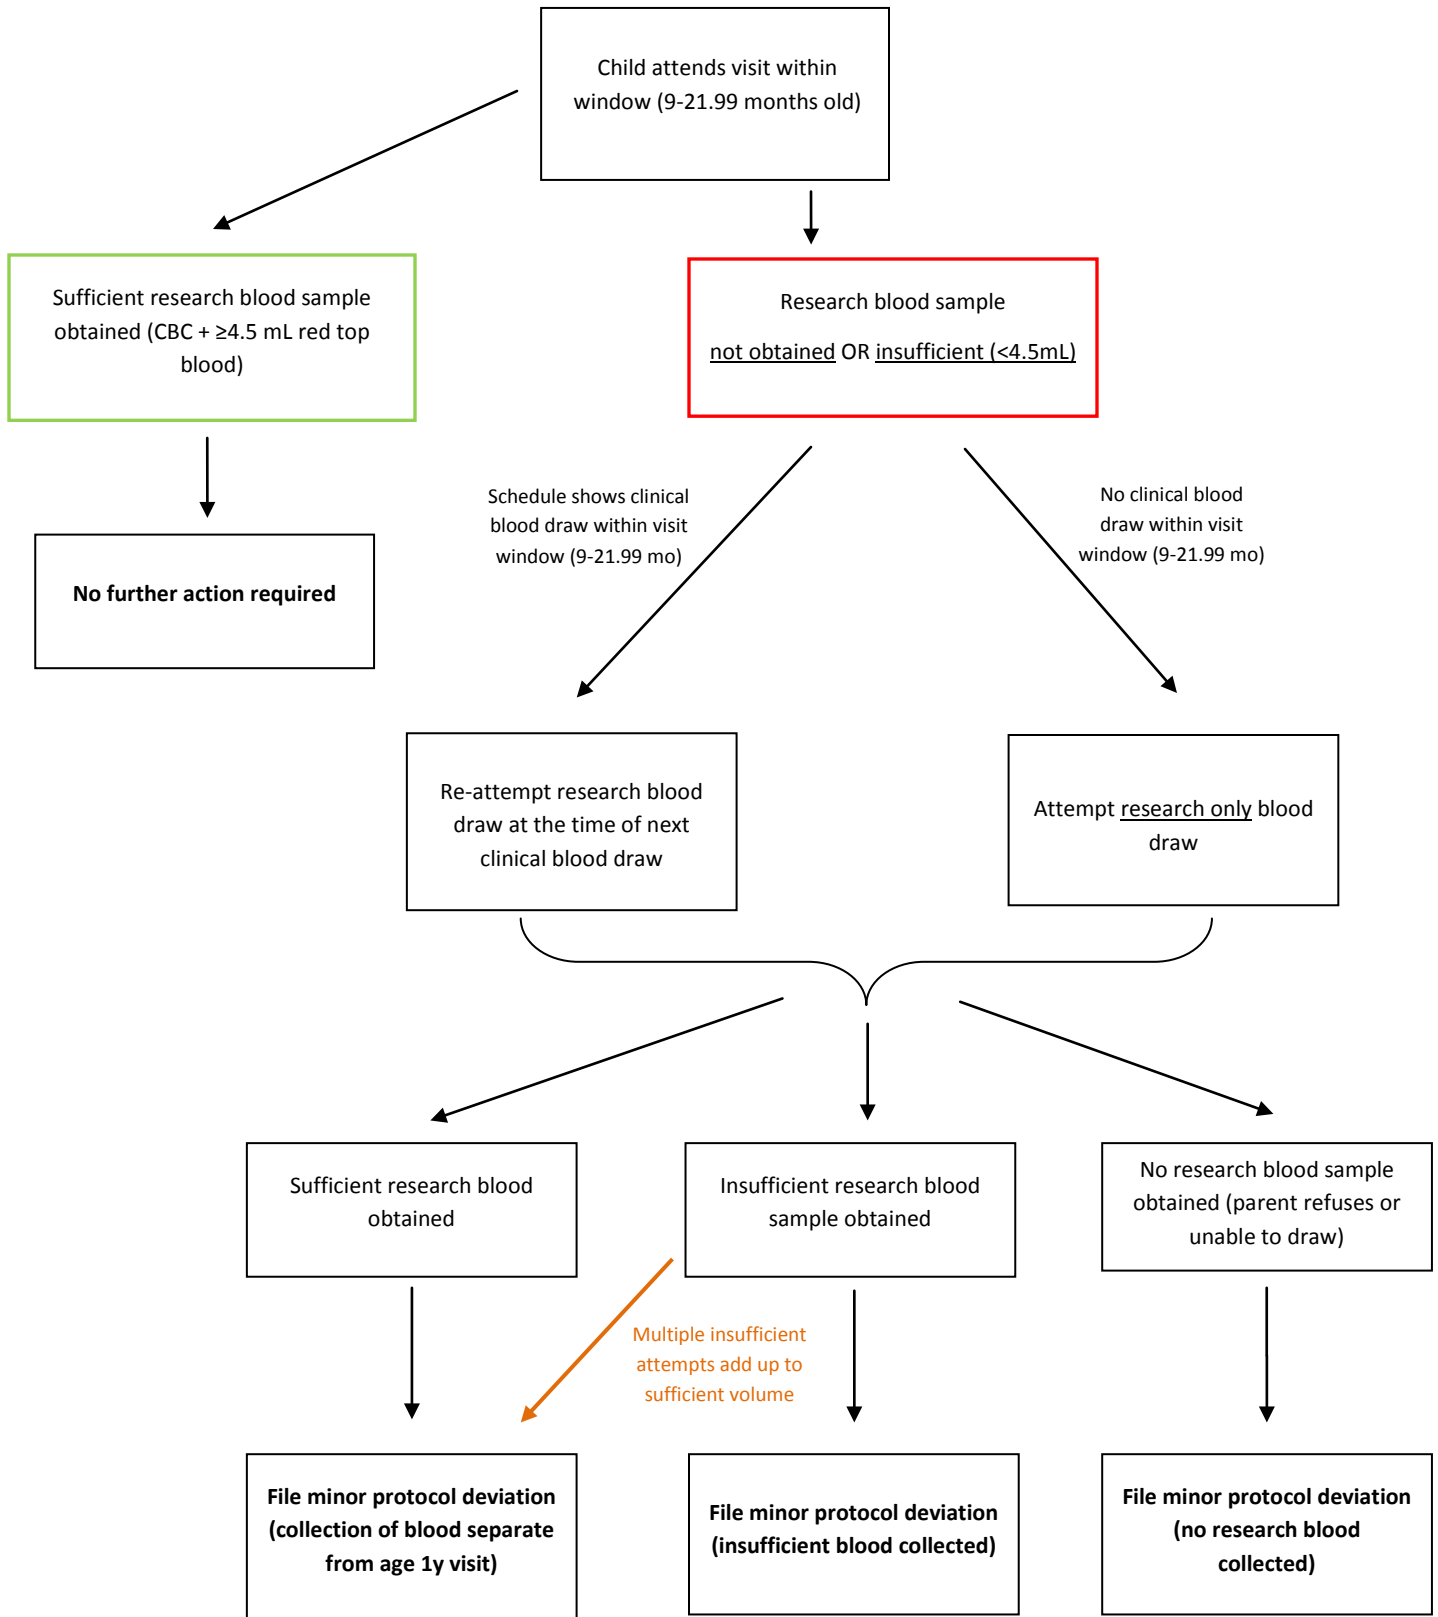

NOTE: The total blood volume collected for each participant per visit should not exceed 15mL, per protocol.